


Example of graph and table of the measured values of the coefficient of absorption of the calibration sample:

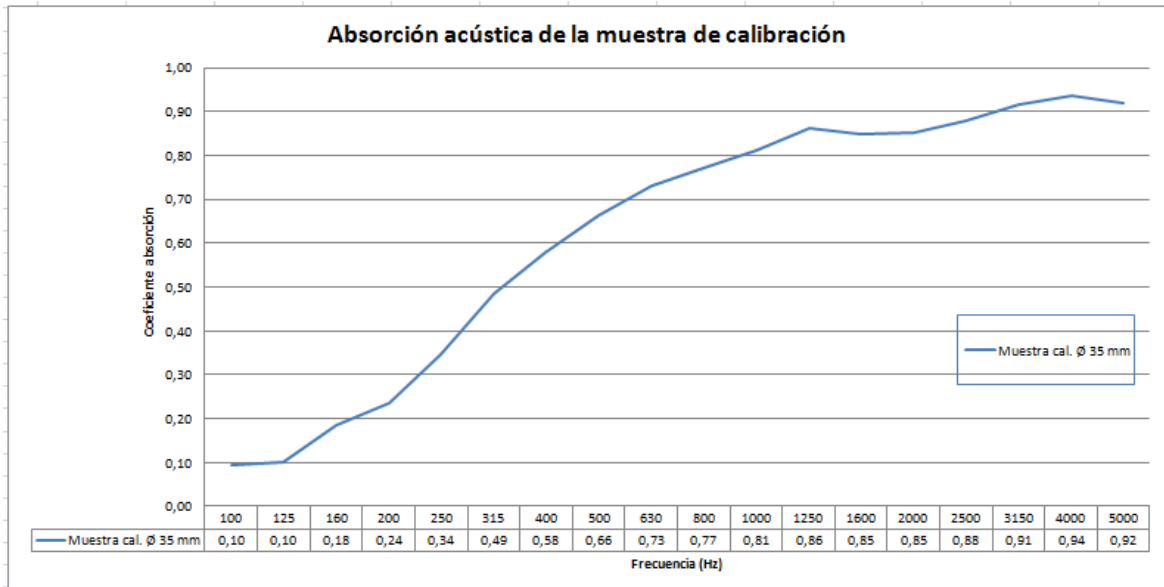

\* When use more than one tube give the measured values of the coefficient of absorption of each calibration sample.